



### Third Committee Draft (3CD) – Marked version

Project: Revision of R 16-1:2002 (*see BIML note on p3*)  
Title: R xxx *Non-invasive non-automated sphygmomanometers*  
*Part 1: Metrological and technical requirements*

Date: 27 September 2019  
Document number: TC18\_SC1\_P1\_N016  
Supersedes document: TC18\_SC1\_P1\_N010

Project Group: OIML TC 18/SC 1/p 1  
Convenership: P.R. China  
Conveners: Ms. Can Wang

Circulated to P- and O-members and liaison international bodies and external organizations for:

☐ ☐ Discussion at (date and place of meeting):

☐ ☐ Comments by:

☐ ☒ Vote (P-members only) and comments by: **27 December 2019**

## Explanatory note

According to OIML B 6 *Directives for OIML technical work*, OIML publications shall be reviewed every five years after publication by the responsible TC/SC to decide whether they should be confirmed, revised, or withdrawn. The current (old) R 16, which TC 18/SC 1 is responsible for, was published in 2002, and it has been identified that there are a few technical conflicts between the new ISO/IEC standard and OIML R 16. To avoid different requirements worldwide on blood pressure instruments, the convener started the work on drafting R 16-1 *Non-invasive mechanical sphygmomanometers* after the project for revision was approved at the 43rd CIML Meeting held in October 2008 in Sydney.

During this work, the convener received dozens of comments from the Project Group's members and liaisons. Therefore, we wish to express our most sincere thanks for all experts' kindness. Many of these proposals have been accepted and published in this current version.

The main changes proposed to R 16-1 are the following:

- OIML R16-1 should be revised into three parts according to OIML B 6, and now OIML Rxxx-1 refers to *Part 1 – Metrological and technical requirements*;
- “*Mechanical sphygmomanometers*” has been replaced by “*Non-automated sphygmomanometers*” to clarify the main distinction between types of sphygmomanometers. This is also an argument consistent with the new ISO/IEC standards;
- Those terms that are no longer used have been deleted;
- “A manual system for applying and releasing pressure” has been replaced by “a pneumatic system” to harmonise the term and also to allow for electro-mechanical control;
- The metrological requirements on MPEs no longer distinguish between “the first time” and “in use”, and the value has finally been set at “0.4 kPa (3 mmHg)” in consideration of recent technical developments in health care;
- In consideration of environmental and health protection, the requirement on the internal diameter of the mercury tube has been deleted to encourage the reduction of the total mercury volume;
- Parts of safety requirements are clarified in agreement with, or according to, the new ISO/IEC standards;
- Verification no longer distinguish between “initial” and “subsequent”;

The current document is the third Committee Draft (3CD). It was drawn up on the basis of the comments received from PG members on the second Committee Draft circulated in December 2018.

Definitions and references related to the International Vocabulary of Metrology – Basic and general concepts and associated terms (VIM) have been modified according to the 2012 edition.

## **BIML note**

The existing R 16 is published in two parts:

R 16-1 *Non-invasive mechanical sphygmomanometers*, and

R 16-2 *Non-invasive automated sphygmomanometers*.

These are being revised under two separate projects: TC 18/SC 1/p 1 and TC 18/SC 1/p 2 respectively.

The existing part numbering of R 16 is not consistent with current OIML practice. All Recommendations are now published with separate parts for the metrological and technical requirements (designated R xxx-1), test procedures (designated R xxx-2), and test report format (designated R xxx-3). To avoid confusion with the existing numbering of R 16, on completion of the two projects, the existing R 16-1 and R 16-2 will be replaced by two separate Recommendations with new numbers and each having three parts:

R xxx-1 *Non-invasive non-automated sphygmomanometers – Metrological and technical requirements*

R xxx-2 *Non-invasive non-automated sphygmomanometers – Test procedures*

R xxx-3 *Non-invasive non-automated sphygmomanometers – Test report format*

R yyy-1 *Non-invasive automated sphygmomanometers – Metrological and technical requirements*

R yyy-2 *Non-invasive automated sphygmomanometers – Test procedures*

R yyy-3 *Non-invasive automated sphygmomanometers – Test report format*

This CD has been re-numbered in line with this arrangement.

## Contents

Foreword.....	6
1. Scope.....	7
2. Terminology.....	7
2.1 Auscultatory method.....	7
2.2 Bladder.....	7
2.3 Cuff.....	7
2.4 Deflation valve.....	7
2.5 Manometer.....	7
2.6 Non-invasive Non-automated sphygmomanometer.....	8
2.7 Non-invasive blood pressure measurement.....	8
2.8 Pneumatic system.....	8
2.9 Rapid exhaust valve.....	8
2.10 Sleeve.....	8
2.11 Tamper proofing.....	9
3. Description of the category of instrument.....	9
4. Units of measurement.....	9
5. Metrological requirements.....	9
5.1 Maximum permissible errors of the cuff pressure indication under ambient conditions.....	9
5.2 Maximum permissible errors of the cuff pressure indication under storage conditions.....	9
5.3 Maximum permissible errors of the cuff pressure indication under varying temperature conditions.....	10
6. Technical requirements.....	10
6.1 Technical requirements for the cuff and bladder.....	10
6.2 Technical requirements for the pneumatic system.....	10
6.3 Technical requirements for the pressure indicating devices.....	10
6.4 Additional technical requirements for mercury manometers.....	12
6.5 Additional technical requirements for aneroid manometers.....	12
6.6 Safety requirements.....	13
6.7 Durability of markings.....	14
7. Metrological controls.....	15
7.1 Type approval.....	15
7.2 Verification.....	15
7.3 Sealing.....	15
7.4 Marking of the device.....	15
7.5 Manufacturer's information.....	16
Annex A: Advice to be included in the instructions accompanying a sphygmomanometer using a mercury manometer.....	17
Foreword.....	5
1. Scope.....	6
2. Terminology.....	6
2.1 Non-automated sphygmomanometer.....	6
2.2 Non-invasive blood pressure measurement.....	6
2.3 Pneumatic system.....	6
2.4 Cuff.....	6

2.5	<u>Bladder</u> .....	6
2.6	<u>Sleeve</u> .....	6
2.7	<u>Deflation valve</u> .....	7
2.8	<u>Auscultatory method</u> .....	7
2.9	<u>Rapid exhaust valve</u> .....	7
2.10	<u>Tamper proofing</u> .....	7
3.	<u>Description of the category of instrument</u> .....	7
4.	<u>Units of measurement</u> .....	7
5.	<u>Metrological requirements</u> .....	7
5.1	<u>Maximum permissible errors of the cuff pressure indication under ambient conditions</u> .....	7
5.2	<u>Maximum permissible errors of the cuff pressure indication under storage conditions</u> .....	7
5.3	<u>Maximum permissible errors of the cuff pressure indication under varying temperature conditions</u> .....	8
6.	<u>Technical requirements</u> .....	8
6.1	<u>Technical requirements for the cuff and bladder</u> .....	8
6.2	<u>Technical requirements for the pneumatic system</u> .....	8
6.3	<u>Technical requirements for the pressure indicating devices</u> .....	8
6.4	<u>Additional technical requirements for mercury manometers</u> .....	10
6.5	<u>Additional technical requirements for aneroid manometers</u> .....	10
6.6	<u>Safety requirements</u> .....	11
7.	<u>Metrological controls</u> .....	12
7.1	<u>Type approval</u> .....	13
7.2	<u>Verification</u> .....	13
7.3	<u>Sealing</u> .....	13
7.4	<u>Marking of the device</u> .....	13
7.5	<u>Manufacturer's information</u> .....	13
	<u>Annex A: Advice to be included in the instructions accompanying a sphygmomanometer using a mercury manometer</u> .....	15

---

## Foreword

The International Organization of Legal Metrology (OIML) is a worldwide, intergovernmental organization whose primary aim is to harmonize the regulations and metrological controls applied by the national metrological services, or related organizations, of its Member States. The main categories of OIML publications are:

**International Recommendations (OIML R)**, which are model regulations that establish the metrological characteristics required of certain measuring instruments and which specify methods and equipment for checking their conformity; the OIML Member States shall implement these Recommendations to the greatest possible extent;

**International Documents (OIML D)**, which are informative in nature and intended to improve the work of the metrological services;

**International Basic Publications (OIML B)**, which define the operating rules of the various OIML structures and systems;

**International Guides (OIML G)**, which are informative in nature and which are intended to give guidelines for the application of certain requirements to legal metrology.

OIML Draft Recommendations, Documents and Guides are developed by Technical Committees or Subcommittees which are formed by the Member States. Certain international and regional institutions also participate on a consultation basis. Cooperative agreements are established between the OIML and certain institutions, such as ISO and the IEC, with the objective of avoiding contradictory requirements; consequently, manufacturers and users of measuring instruments, test laboratories, etc. may simultaneously apply OIML publications and those of other institutions.

International Recommendations, Documents and Guides are published in French (F) and English (E) and are subject to periodic revision.

Additionally, the OIML participates in the publication of **Vocabularies (OIML V)** and periodically commissions legal metrology Experts to write **Expert Reports (OIML E)**. Expert Reports are intended to provide information and advice to metrological authorities, and are written solely from the viewpoint of their author, without the involvement of a Technical Committee or Subcommittee, nor that of the CIML. Thus they do not necessarily represent the views of the OIML.

This publication - reference OIML R 16-1, edition **201X (E)** - was developed by the OIML Technical Subcommittee TC 18/SC 1 Blood pressure instruments. It was approved for final publication by the International Committee of Legal Metrology in **201X** and supersedes OIML R 16-1:2002 (E).

OIML Publications may be downloaded from the OIML web site in the form of PDF files. Additional information on OIML Publications may be obtained from the Organization's headquarters:

Bureau International de Métrologie Légale

11, rue Turgot - 75009 Paris - France

Telephone: 33 (0)1 48 78 12 82

Fax: 33 (0)1 42 82 17 27

E-mail: biml@oiml.org

# Non-invasive Non-automated Sphygmomanometers

## Part 1: Metrological and technical requirements

### 1. Scope

This Recommendation specifies general, performance, efficiency— and mechanical ~~and electrical~~ safety requirements, including test methods for type approval, for non-invasive, non-automated sphygmomanometers and their accessories which, by means of an inflatable cuff, are used for the non-invasive measurement of arterial blood pressure. ~~The application of the cuff is not limited to a particular extremity of the human body (e.g. the upper arm)~~

Included within the scope of this Recommendation are non-invasive non-automated sphygmomanometers with a mechanical or integrated electro-mechanical pressure sensing element and display, used in conjunction with a stethoscope or other manual methods for detecting Korotkoff sounds and for cuff inflation.

### 2. Terminology

#### 2.1 Auscultatory method

~~M~~method whereby sounds (known as Korotkoff sounds) are heard or detected (e.g. by a microphone) over an occluded artery as the occluding pressure is slowly released, the appearance of sounds coinciding with the systolic blood pressure and the disappearance of sounds with the diastolic blood pressure.

#### 2.2 Bladder

~~i~~Inflatable component of the cuff.

#### 2.3 Cuff

~~C~~component of the non-invasive non-automated sphygmomanometer, comprising a bladder and a sleeve, which is wrapped around the limb of the patient.

#### 2.4 Deflation valve

~~V~~valve for controlled exhaust of the pneumatic system during measurement.

#### 2.5 Diastolic blood pressure (value)

~~M~~minimum value of the arterial blood pressure as a result of relaxation of the systemic ventricle.

Note: Because of hydrostatic effects, this value should be measured with the cuff at the heart level.

#### 2.6 Manometer

~~I~~nstrument used to measure and display pressure.

## ~~2.7~~ ~~2.1~~ — ~~Non-invasive~~ ~~Non-automated~~ sphygmomanometer

~~Sphygmomanometer which allows a trained person to use an inflatable cuff for the non invasive measurement estimation of the arterial blood pressure by means of the cuff pressure display. (See also Note under 3.)~~  
~~Device used by a trained person for the non-invasive measurement of the arterial blood pressure by utilizing an inflatable cuff with a display and used in conjunction with a stethoscope for measuring the arterial blood pressure. hereafter is named sphygmomanometer in this recommendation.~~

## ~~2.8~~ ~~2.2~~ — Non-invasive blood pressure measurement

~~Indirect measurement of the arterial blood pressure without arterial puncture.~~

## ~~2.9~~ ~~2.3~~ — Pneumatic system

~~System that includes all pressurized and pressure-controlling parts such as cuff, tubing, connectors, valves, transducer and pump.~~

## ~~2.4~~ Cuff

~~Component of the sphygmomanometer, comprising a bladder and a sleeve, which is wrapped around the limb of the patient.~~

## ~~2.5~~ Bladder

~~Inflatable component of the cuff.~~

## ~~2.10~~ Rapid exhaust valve

~~Valve for rapidly exhausting the pneumatic system.~~

## ~~2.11~~ ~~2.6~~ — Sleeve

~~Essentially inelastic part of the cuff that encloses the bladder.~~

## ~~2.12~~ Systolic blood pressure (value)

~~Maximum value of the arterial blood pressure as a result of the contraction of the systemic ventricle.~~

~~Note: Because of hydrostatic effects, this value should be measured with the cuff at the heart level.~~

## ~~2.7~~ Deflation valve

~~Valve for controlled exhaust of the pneumatic system during measurement.~~

## ~~2.8~~ Auscultatory method

~~Technique whereby sounds (known as Korotkoff sounds) are heard over an occluded artery as the occluding pressure is slowly released, the appearance of sounds coinciding with the systolic blood pressure and the disappearance of sounds with the diastolic blood pressure in adults. In children under age of 13, “k4” (i.e. 4th phase Korotkoff sound) may be appropriate.~~

## ~~2.9~~ Rapid exhaust valve

~~Valve for rapidly exhausting the pneumatic system.~~



### **2.13 ~~2.10~~—Tamper proofing**

~~Means of preventing the user from gaining easy access to the measuring mechanism of the device.~~

## **3. Description of the category of instrument—**

~~The basic components of a sphygmomanometer are a cuff that can be wrapped around a patient's limb, a pneumatic system for applying and releasing pressure in the bladder, and a means of measuring and displaying the instantaneous pressure in the bladder.~~

~~Non-automated sphygmomanometers typically use either a mercury or an aneroid manometer or another mechanical measuring device for the non-invasive measurement of the arterial blood pressure by means of an inflatable cuff.~~

~~*Note:*—Components of these devices are manometer, cuff, valve for deflation (often in combination with rapid exhaust valve), hand pump or electromechanical pump and connection hoses. These devices may also contain electro-mechanical components for pressure control. The basic components of a sphygmomanometer are a manometer for measuring and displaying pressure in the bladder and a pneumatic system for applying and releasing pressure in the bladder.~~

~~Pneumatic system includes cuff that can be wrapped around a patient's limb, tubing, connectors, valve for deflation (often in combination with rapid exhaust valve), transducers and hand pump or electromechanical pump. For pressure control, electro-mechanical components may be used.~~

~~Sphygmomanometers typically use either a mercury or an aneroid manometer or another mechanical measuring device for the non-invasive measurement of the arterial blood pressure by means of an inflatable cuff.~~

## **4. Units of measurement**

The blood pressure shall be indicated either in kilopascal (kPa) or in millimeter of mercury (mmHg).

## **5. Metrological requirements**

### **5.1 Maximum permissible errors of the cuff pressure indication under ambient conditions**

For any set of conditions within the ambient temperature range ~~of from~~ 15 °C to 25 °C and the relative humidity range ~~of from~~ 15 % to 85 % for decreasing pressure, the maximum permissible error for the measurement of the cuff pressure at any point of the scale range shall be ~~±0.4 kPa (±3 mmHg)~~ for sphygmomanometers.

### **5.2 Maximum permissible errors of the cuff pressure indication under storage conditions**

The sphygmomanometer without electronic components shall maintain the maximum permissible error requirements for the measurement of the cuff pressure specified in this Recommendation (5.1) after a storage for 24 h at a low temperature of ~~−20 °C~~ and which is followed by an additional storage for 24 h at a high temperature of 70 °C and at a relative humidity of 85 % (non-condensing).

The sphygmomanometer with electronic components shall maintain the maximum permissible error requirements for the measurement of the cuff pressure specified in this Recommendation (5.1) after a storage for 24 h at a low temperature of -5 °C ~~and which is followed by an additional storage~~ for 24 h at a high temperature of 50 °C and at a relative humidity of 85 % (non-condensing).

The ~~test~~storage shall ~~be performed~~occur with the unpacked sphygmomanometers.

### 5.3 Maximum permissible errors of the cuff pressure indication under varying temperature conditions

For the ambient temperature range ~~of from~~ 10 °C-°C to 40 °C-°C and the relative humidity of 85 % (non-condensing), the difference between the indicated pressure of the manometer of the device to be tested and the corresponding readings of the reference manometer ~~(see B.4)~~ at the relevant temperature value shall not exceed  $\pm 0.4$  kPa ( $\pm 3$  mmHg) or  $\pm 2$  % of the reading, whichever is greater.

*Note* ~~+~~ -: The requirement of this subclause does not apply to mercury manometers.

## 6. Technical requirements

### 6.1 Technical requirements for the cuff and bladder

The cuff shall contain a bladder. For reusable cuffs the manufacturer shall indicate the method for cleaning in the accompanying documents (see 7.5).

The bladder length should be approximately 0.80 ~~×~~ the circumference of the limb at the midpoint of the intended range of the cuff. The width of the bladder should be at least 0.40 ~~×~~ the circumference of the limb at the midpoint of the intended range of the cuff.

### 6.2 Technical requirements for the pneumatic system

#### 6.2.1 Air leakage

Air leakage shall not exceed a pressure drop of 0.5 kPa/min (4 mmHg/min).

#### 6.2.2 Pressure reduction rate

The deflation valves in the pneumatic system shall be capable of adjustment to a deflation rate from 0.3 kPa/s to 0.4 kPa/s (2 mmHg/s to 3 mmHg/s).

The deflation valves in the pneumatic system shall be easily adjusted to these values.

#### 6.2.3 Rapid exhaust

During the rapid exhaust of the pneumatic system, with the valve fully opened, the time for the pressure reduction from 35 kPa to 2 kPa (260 mmHg to 15 mmHg) shall not exceed 10 s.

### 6.3 Technical requirements for the pressure indicating devices

#### 6.3.1 Nominal range and measuring range

The nominal range shall be equal to the measuring range.

The nominal range for the cuff pressure indication shall extend from 0 kPa to at least 35 kPa (0 mmHg to at least 260 mmHg).

### 6.3.2 Analogue indication

#### 6.3.2.1 Scale

The scale shall be designed and arranged so that the measuring values can be read clearly and are easily recognized.

Testing shall be carried out by visual inspection.

#### 6.3.2.2 First scale mark

The graduation shall begin with the first scale mark at 0 kPa (0 mmHg).

Testing shall be carried out by visual inspection.

#### 6.3.2.3 Scale interval

The scale interval shall be:

- 0.5 kPa for a scale graduated in kPa;
- 2 mmHg for a scale graduated in mmHg.

In the case ~~for of~~ a scale graduated in kPa: Each ~~second-fourth~~ scale mark shall be indicated by greater length and each ~~fourth-eighth~~ scale mark shall be numbered. In the case ~~for of~~ a scale graduated in mmHg: Each fifth scale mark shall be indicated by greater length and each tenth scale mark shall be numbered. An example of a scale in mmHg is given in Figure 1.

For sphygmomanometers with a manometer with elastic or electro-mechanical sensing elements, no graduation is needed within the range ~~of from~~ > 0 kPa to < 2 kPa (> 0 mmHg to < 15 mmHg).

Testing shall be carried out by visual inspection.

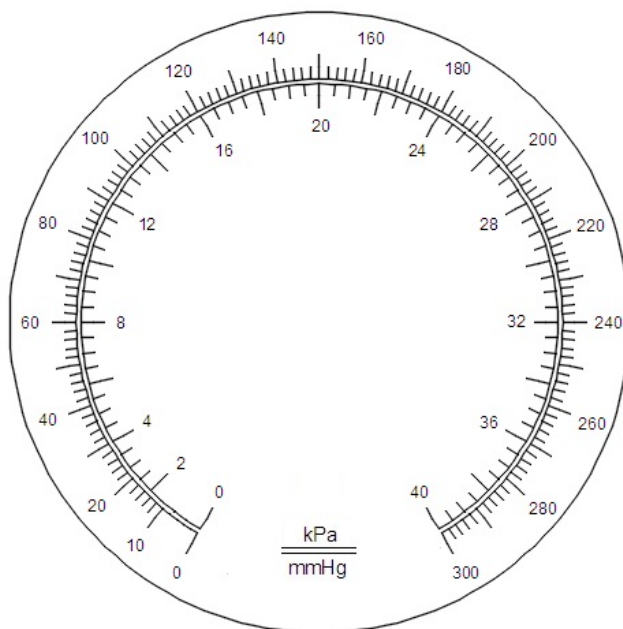


Figure 1 Example of an aneroid manometer scale  
(division in mmHg without a tolerance zone at zero)

#### 6.3.2.4 Scale spacing and thickness of the scale marks

The distance between adjacent scale marks shall be not less than 1.0 mm. The thickness of the scale marks shall not exceed 20% of the smallest scale spacing.

All scale marks shall be of equal thickness.

#### 6.3.3 Digital indication

The digital scale interval shall be 0.1 kPa (1 mmHg).

If the measured value of a parameter is to be indicated on more than one display, all the displays shall indicate the same numerical value.

Measured numerical values on the display(s), and the symbols defining the units of measurement shall be arranged in such a way so as to avoid misinterpretation.

Numbers and characters should be clearly legible.

Testing shall be carried out by visual inspection.

### 6.4 Additional technical requirements for mercury manometers

#### 6.4.1 Portable devices

A portable device shall be provided with an adjusting or locking mechanism to secure it in the specified position of use.

Testing shall be carried out by visual inspection.

#### 6.4.2 Devices to prevent mercury from being spilled during use and transport

A device shall be placed in the tube to prevent mercury from being spilled during use and transport (for example: stopping device, locking device, etc.). This device shall be such that when the pressure in the system drops rapidly from 27 kPa to 0 kPa (from 200 mmHg to 0 mmHg), the time taken for the mercury column to fall from 27 kPa to 5 kPa (from 200 mmHg to 40 mmHg) shall not exceed 1.5 s. This time is known as the "exhaust time".

#### 6.4.3 Quality of the mercury

6.4.3.1 The mercury shall have a purity of not less than 99.99% according to the declaration of the supplier of the mercury.

6.4.3.2 The mercury shall exhibit a clean meniscus and shall not contain air bubbles.

#### 6.4.4 Graduation of the mercury tube

Graduations shall be permanently marked on the tube containing mercury. If numbered at each fifth scale mark, the numbering shall be alternately on the right- and left-hand side of, and adjacent to, the tube.

Testing shall be carried out by visual inspection.

### 6.5 Additional technical requirements for aneroid manometers

#### 6.5.1 Scale mark at zero

If a tolerance zone is shown at zero it shall not exceed  $\pm 0.4$  kPa ( $\pm 3$  mmHg) and shall be clearly marked. A scale mark at zero shall be indicated.

*Note:* Graduations within the tolerance zone are optional.

Testing shall be carried out by visual inspection.

### 6.5.2 Zero

The movement of the elastic sensing element including the pointer shall not be obstructed within 0.8 kPa (6 mmHg) below zero.

Neither the dial nor the pointer shall be adjustable by the user.

Testing shall be carried out by visual inspection.

### 6.5.3 Pointer

The pointer shall cover between 1/3 and 2/3 of the length of the shortest scale mark of the scale. At the place of ~~indication~~indication, it shall be not thicker than the scale mark. The distance between the pointer and the dial shall not exceed 2 mm.

~~Testing shall be carried out by visual inspection.~~

### 6.5.4 Hysteresis error

The hysteresis error throughout the pressure range shall not exceed the range 0 kPa to 0.5 kPa (0 mmHg to 4 mmHg).

### 6.5.5 Durability of manometer

The construction of the manometer and the material for the elastic sensing elements shall ensure an adequate stability of the measurement. When elastic sensing elements are used, they shall be aged with respect to pressure and temperature. After 10 000 alternating pressure cycles from 3 kPa (20 mmHg) to full scale, the change in the pressure indication shall be not more than 0.4 kPa (3 mmHg) ~~throughout the pressure range~~.

## 6.6 Safety requirements

### 6.6.1 Mechanical safety

#### 6.6.1.1 Resistance to shock for handheld sphygmomanometers

~~Non-automated sphygmomanometers~~ Sphygmomanometers or their parts shall have adequate mechanical strength when subjected to mechanical stress caused by normal use, pushing, impact, dropping and rough handling.

Wall mounted ~~non-automated~~ sphygmomanometers and mercury manometers are exempt from the requirements of this subclause.

~~The non-automated sphygmomanometer~~ Sphygmomanometers shall function normally following a free fall from a distance  $d=25$  cm.

A ~~non-automated~~ sphygmomanometer that is marked “Shock Resistant” shall function normally following a free fall from a distance  $d=1$  m.

Allow the ~~non-automated~~ sphygmomanometer to fall freely ~~six~~ 6 times (once on each side) from a height of distance  $d_1$  onto a  $50 \pm 5$  mm thick hardwood (hardwood density  $> 600$  kg/m<sup>3</sup>) board lying flat on a concrete or a similar rigid base.

After testing, the device shall comply with the requirements of 5.1.

#### 6.6.1.2 ~~Non-automated~~ sphygmomanometers used during patient transport

~~Non-automated sphygmomanometers~~ Sphygmomanometers or their parts, intended for use during patient transport outside a healthcare facility, shall have adequate mechanical strength when subjected to mechanical stress caused by normal use, pushing, impact, dropping, and rough handling.

a) Shock:

- Peak acceleration: 1\_000 m/s<sup>2</sup> (10<sup>2</sup>\_g)
- Duration: 6\_ms
- Pulse shape: Half sine
- Number of shocks: ~~3~~three shocks per direction per axis (18 total)

b) Broad-band random vibration:

- Frequency range: 10\_Hz to 2000\_Hz
- Resolution: 10\_Hz
- Acceleration amplitude:
  - 10\_Hz to 100\_Hz: 5.0\_(m/s<sup>2</sup>)<sup>2</sup>/Hz
  - 100\_Hz to 200\_Hz: ~~-7~~\_db/octave
  - 200\_Hz to 2000\_Hz: 1.0\_(m/s<sup>2</sup>)<sup>2</sup>/Hz
- Duration: 30 min per each perpendicular axis (~~3~~three total)

After testing, the device shall comply with the requirements of 5.1.

6.6.1.3 ~~Non-automated sphygmomanometers~~ Sphygmomanometers containing a mercury manometer

A ~~non-automated~~ sphygmomanometer containing a mercury manometer shall not leak mercury following a free fall from a distance  $d=1\_m$ .

Allow the ~~non-automated~~ sphygmomanometer to fall freely ~~6~~six times (once on each side) from a height of distance  $d$  onto a  $50\_mm \pm 5\_mm$  thick hardwood (hardwood density  $> 600\_kg/m^3$ ) board lying flat on a concrete or a similar rigid base. Care should be taken while testing to ensure that there is no escape of mercury into the environment should the ~~non-automated~~ sphygmomanometer under test fail. After the test, visually inspect to check that there is no leakage of mercury from the manometer of the ~~non-automated~~ sphygmomanometer.

After testing, the device shall comply with the requirements of 5.1.

6.6.2 *Abort a measurement*

It shall be possible to abort the blood pressure measurement at any time by activating the manual rapid exhaust valve, which shall be easily accessible.

6.6.3 *Tamper proofing*

Means shall be provided to prevent tampering or unauthorized access:

- for all ~~non-automated~~ sphygmomanometers, any adjustment or function that affects accuracy;
- for mercury ~~non-automated~~ sphygmomanometers, the separation of reservoir and scale.

EXAMPLE: Requiring a tool for opening or seal breakage.

It shall be clear to an operator if tampering or unauthorized access has occurred.

6.6.4 *Electrical safety*

Regional or national regulations may specify electrical safety requirements.

6.6.5 *Tubing connectors*

Luer lock and Luer slip connectors shall not be used on non-automated sphygmomanometers so as to avoid any risk of connecting the output of the ~~non-automated~~ sphygmomanometer to intravascular fluid systems as air might inadvertently be pumped into a blood vessel.

**6.7 Durability of markings**

The markings required shall be removable only with a tool or by appreciable force and shall be sufficiently

durable to remain clearly legible during the expected service life of the sphygmomanometer. In considering the durability of the markings, the effect of normal use shall be taken into account.

## 7. Metrological controls

Regional or national regulations may prescribe type approval, initial and/or subsequent verification for ~~noninvasive~~-sphygmomanometers. These metrological controls shall meet the following conditions.

### 7.1 Type approval

At least three samples of a new type of sphygmomanometer shall be tested.

The tests to verify conformity to metrological and technical requirements shall be carried out according to OIML ~~R16~~Rxxx-2. A test report shall be prepared according to OIML ~~R16~~Rxxx-3.

### 7.2 Verification

After type approval has been granted, verification shall be carried out before the ~~non-automated~~ sphygmomanometer is put into use and during its lifetime. At verification, testing can be conducted at any set of climatic conditions within the temperature range ~~offrom~~ 15 °C to 25 °C and the relative humidity range ~~fromof~~ 15 % to 85 %. A climatic chamber is not required.

Each instrument of an approved type of ~~non-automated~~ sphygmomanometer shall be verified periodically in accordance with applicable metrological laws and regulations of a member state, or after repair. At least the requirements of 5.1 and 6.2.1 shall be fulfilled.

### 7.3 Sealing

7.3.1 Control marks will be put on lead seals for which corresponding punched screws shall be attached whenever necessary. These seals shall prevent, without destruction of the control marks:

- in the case of mercury manometers: the separation of reservoir and scale;
- in the case of all other manometers: the opening of the casing.

7.3.2 If the construction of the instrument guarantees security against any interference, the metrological control marks or the security marks may be attached in form of labels.

7.3.3 All seals shall be accessible without using a tool.

### 7.4 Marking of the device

The ~~devices~~sphygmomanometer shall be marked with the following information:

- ~~• name and/or trademark of manufacturer;~~
  - ~~• serial number and year of fabrication;~~
  - ~~• measuring unit;~~
  - ~~• type approval number (if applicable);~~
  - ~~• on the cuff an indication of the correct positioning for the cuff over the artery;~~
  - ~~• on the cuff an indication of the limb circumference for which it is appropriate (see 6.1);~~
  - ~~• information for containing mercury are required for mercury manometers.~~
- 7.4.1 On the indicating device
- name and/or trademark of manufacturer;
  - type of sphygmomanometer;
  - units of measurement (kPa/mmHg), positioned close to the displayed values;

- measuring range;
- type approval number (if applicable);
- serial number;
- year of fabrication;
- country of origin;
- information for containing mercury are required for mercury manometers.

#### 7.4.2 On the cuff

- limb circumference for which it is appropriate;
- marking of the limb circumference indication range;
- center of the bladder, indicating the correct position for the cuff over the artery.

### 7.5 Manufacturer's information

Information supplied by the manufacturer shall comply with the specifications and requirements given in this Recommendation.

The manufacturer's instruction manual shall contain the following information:

- reference to OIML R ~~16xxx~~, including the complete title;
- explanation of the operating procedures which are important for correct application (such as the selection of the appropriate cuff size, positioning of the cuff at the heart level and adjustment of the pressure reduction rate);
- methods for cleaning reusable cuffs;
- if the bladder is removable, the method for ensuring the correct repositioning of the bladder in the cuff;
- nature and frequency of the maintenance is required to ensure that the device operates correctly and safely at all times; a disclosure that applicable national or regional metrological laws and regulations ~~have to be taken into account~~ shall be considered;
- detailed instructions for the safe handling of mercury (see Annex A);
- a list of all components belonging to the pressure measuring system, including accessories;
- remarks on the environmental or operational factors which may affect the performance (e.g. electromagnetic fields, arrhythmia);
- specification of the rated voltage, if applicable;
- specification of the intended power source, if applicable;
- measuring range;
- the operating and storage temperature and humidity ranges;
- warm up time, if applicable;
- description of all symbols, abbreviations and error codes used on the instrument; and
- Name and address of manufacturer.-



## **Annex A: Advice to be included in the instructions accompanying a sphygmomanometer using a mercury manometer**

(Informative)

### **A.1. Guidelines and precautions**

A mercury-type sphygmomanometer should be handled with care. In particular, care should be taken to avoid dropping the instrument or treating it in any way that could result in damage to the manometer. Regular checks should be made to ensure that there are no leaks from the inflation system and to ensure that the manometer has not been damaged so as to cause a loss of mercury.

### **A.2. Health and safety when handling mercury**

Exposure to mercury can have serious toxicological effects; absorption of mercury results in neuropsychiatric disorders and, in extreme cases, of nephrosis. Therefore, precautions should be taken when carrying out any maintenance to a mercury-type sphygmomanometer.

When cleaning or repairing the instrument, it should be placed on a tray having a smooth, impervious surface which slopes away from the operator at about 10° to the horizontal, with a water-filled trough at the rear. Suitable gloves (e.g. of latex) should be worn to avoid direct skin contact. Work should be carried out in a well-ventilated area, and ingestion and inhalation of the vapor should be avoided.

For more extensive repairs, the instrument should be securely packed with adequate padding, sealed in a plastic bag or container, and returned to a specialist repairer. It is essential that a high standard of occupational hygiene is maintained in premises where mercury-containing instruments are repaired. Chronic mercury absorption is known to have occurred in individuals repairing sphygmomanometers.

### **A.3. Mercury spillage**

When dealing with a mercury spillage, wear latex gloves. Avoid prolonged inhalation of mercury vapor. Do not use an open vacuum system to aid collection.

Collect all the small droplets of split mercury into one globule and immediately transfer all the mercury into a container, which should then be sealed.

After removal of as much of the mercury as practicable, treat the contaminated surfaces with a wash composed of equal parts of calcium hydroxide and powdered sulfur mixed with water to form a thin paste. Apply this paste to all the contaminated surfaces and allow to dry. After 24 h, remove the paste and wash the surfaces with clean water. Allow to dry and ventilate the area.

---

#### A.4. Cleaning the manometer tube

To obtain the best results from a mercury-type sphygmomanometer, the manometer tube should be cleaned at regular intervals (e.g. under the recommended maintenance schedule). This will ensure that the mercury can move up and down the tube freely, and respond quickly to changes in pressure in the cuff.

During cleaning, care should be taken to avoid the contamination of clothing. Any material contaminated with mercury should be sealed in a plastic bag before disposal in a refuse receptacle.